



Hach BioTector B3500ul Online TOC Analyzer

Applications

- Dry steam condensate return
- Boiler feed
- Drinking Water from desalination



Precise, low-level TOC measurement that you can trust

Changes in water quality for ultra pure applications are disruptive to plant operations. Accurate, on-line analysis is important to protect critical equipment that depends on ultra pure water resources. Leading manufacturers know that it is critical to analyse for contaminants precisely at ppb levels to maintain water quality. Reliability and effective oxidation of large samples ensures that manufacturers can trust the results reported by the BioTector B3500ul analyzer. With a full picture of organic contaminants in critical water applications manufacturers make water treatment decisions more efficiently.

The Hach® BioTector B3500ul provides reliable and accurate TOC analysis at ppb levels for ultrapure water applications. The patented two stage advanced oxidation technology behind the BioTector thoroughly, and reliably oxidizes samples for valuable real-time water analysis.

Maximum uptime for your process

With uptime certified at 99.86% and two short, scheduled maintenance events per year, you will not be missing critical process information when you need it the most.

Instant and long term savings

Reduce the costs related to water re-treatment, and save on operational expenses. On-line TOC analysis enables maximum water reuse and keeps critical water resources at their best to maximize the lifetime of high-value capital equipment.

Technical Data*

Parameter	TOC, TIC, TC, VOC, after correlation COD, BOD	EExp / Hazardous Location	Certification options are available to European Standards, (ATEX Zone 1, Zone 2), North American Standards (Class I Division 2) and IECEx Zone 1
Measurement Method	Infrared measurement of CO ₂ after oxidation	Sample Inlet Temperature	2 - 60 °C (36 - 140°F)
Oxidation Method	Patented Two-Stage Advanced Oxidation Process (TSAO) using Hydroxyl Radicals	Ambient Temperature	5 - 45 °C (41 - 113 °F) Cooling and heating options are available.
Range	0 - 5000 µg/L C	Humidity	5 - 85 % (non-condensing)
Multi-Stream	Up to 2 process streams and grab sample	Particle Size	Up to 100 µm
Repeatability	± 2% of reading or ± 6 µg/L C, whichever is greater	Data Storage	Previous 9999 analysis data on screen in the microcontroller memory and storage of data archive for the lifetime of the analyzer in the SD/MMC card. Previous 99 fault data on screen in the microcontroller memory and storage of fault data archive for the lifetime of the analyzer in the SD/MMC card.
Accuracy	±2 % of reading or ±15 µg/L C, whichever is greater	Display	High contrast 40 character x 16 line backlit LCD with LED backlight
Limit of quantification	80 µg/L	User Interface	Microcontroller with membrane keyboard
Calibration	For best performance ultra-pure water (18.2 MΩ*cm, < 5 µg/L TOC) is needed for calibration.	Power Requirements (Voltage)	115 V AC/230 V AC
Interferences	TIC Interference: At 500 µg/L TIC (as bicarbonate), 2% carryover into TOC may occur.	Power Requirements (Hz)	50/60 Hz
pH Range	pH 1-12	Service Interval	6 months service intervals
Cycle Time	TOC from 5 minutes, depending on application	Dimensions (H x W x D)	1000 mm x 500 mm x 320 mm
Communication	Modbus RTU, Modbus TCP/IP & Profibus (when the Profibus option is selected, the digital output signals are sent through the Profibus converter with its specific communication protocol) Except for Zone 1 certification then Modbus RTU, Modbus TCP/IP & Modbus TCP/IP Redundant is available	Weight	50 kg
Protection Class	IP44, standard fan cooled, maximum ambient temperature 45 °C IP54, air cooled, maximum ambient temperature 35 °C IP54, vortex cooled, maximum ambient temperature 50 °C		

*Subject to change without notice.

Principle of Operation

TIC

Acid is added to lower the pH so that inorganic carbon is sparged off as CO_2 . This is also measured to ensure the Total Inorganic Carbon (TIC) is not carried over into the TOC.

Oxidation


BioTectors's patented oxidation method (TSAO) efficiently oxidizes the organic carbon in the sample to CO_2 . TSAO utilizes hydroxyl radicals generated within the analyzer by combining oxygen, which passes through the ozone generator, with sodium hydroxide.

TOC

To remove CO_2 from the oxidized sample, the pH of the sample is lowered again. The CO_2 is sparged and measured by the specially developed NDIR CO_2 analyzer. The result is displayed as Total Organic Carbon (TOC).



Dimensions

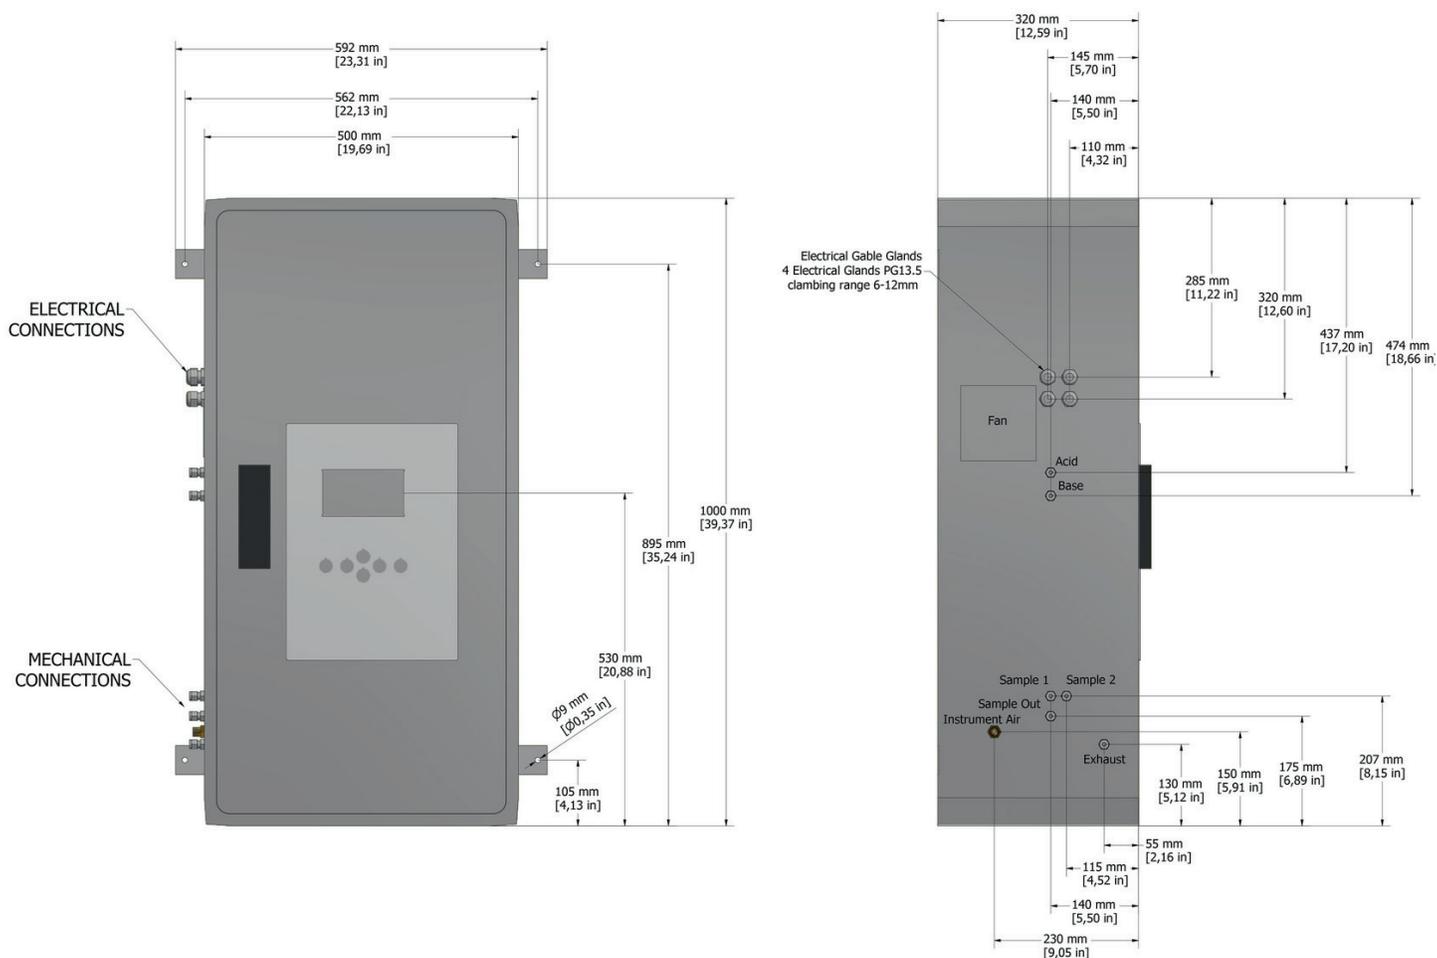

Order Information*

Instruments

B5EBAA152EAC2 Hach BioTector B3500ul TOC analyzer, 0 - 5000 µg/L C, 1 stream, grab sample, 115 V AC

B5EBAA152EAF2 Hach BioTector B3500ul TOC analyzer, 0 - 5000 µg/L C, 2 streams, grab sample, 115 V AC

There are additional options available. Please contact Hach for more details.

Accessories

19-COM-160 BioTector Compressor 115 V / 60 Hz

19-COM-250 BioTector Compressor 230 V / 50 Hz

10-SMC-001 Air supply filter pack

19-KIT-123 Six months spare part kit for BioTector B3500

19-BAS-031 BioTector sample overflow chamber

Reagents

2985562 BioTector base reagent 1.2 N sodium hydroxide

25255061 BioTector acid reagent 1.8 N sulfuric acid containing 80 mg/L Mn

Part numbers may vary by country.

Hach Service Protects Your Investment

With Hach Service, you have a global partner who understands your needs and cares about delivering timely, high-quality service you can trust. Our Service Team brings unique expertise to help you maximize instrument uptime, ensure data integrity, maintain operational stability, and reduce compliance risk.



World Headquarters: Loveland, Colorado USA | [hach.com](https://www.hach.com)

United States 800-227-4224 fax: 970-669-2932 email: orders@hach.com
Outside United States 970-669-3050 fax: 970-461-3939 email: intl@hach.com

©Hach Company, 2024. All rights reserved.

In the interest of improving and updating its equipment, Hach Company reserves the right to alter specifications to equipment at any time.

DOC053.53.35110.Dec24