



## Threshold Setup for Innovate System Win10 Software


1. Launch Innovate V5.25 software.

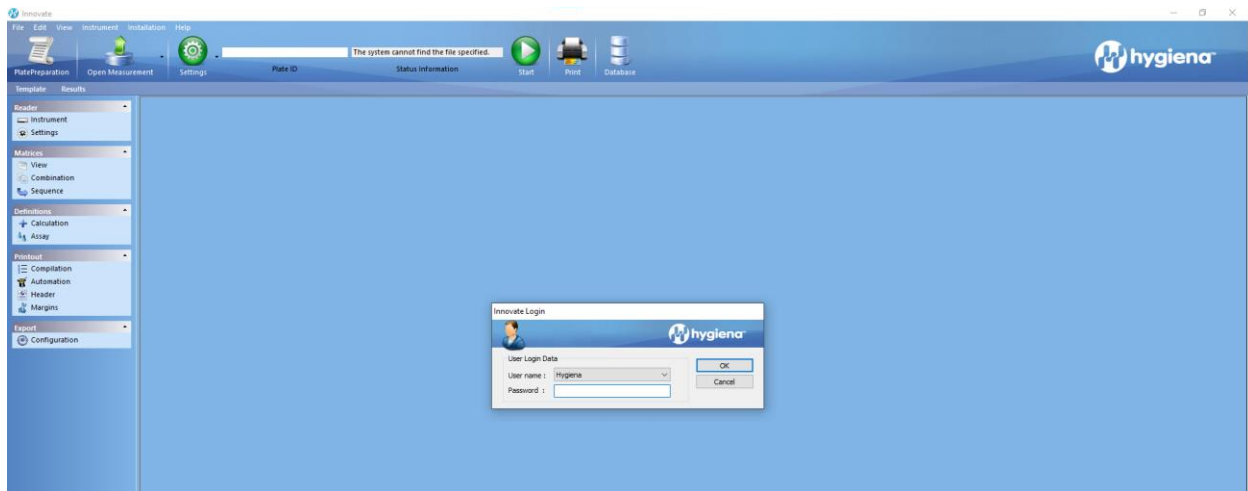


2. Change username to System Manager. Password: **Default**

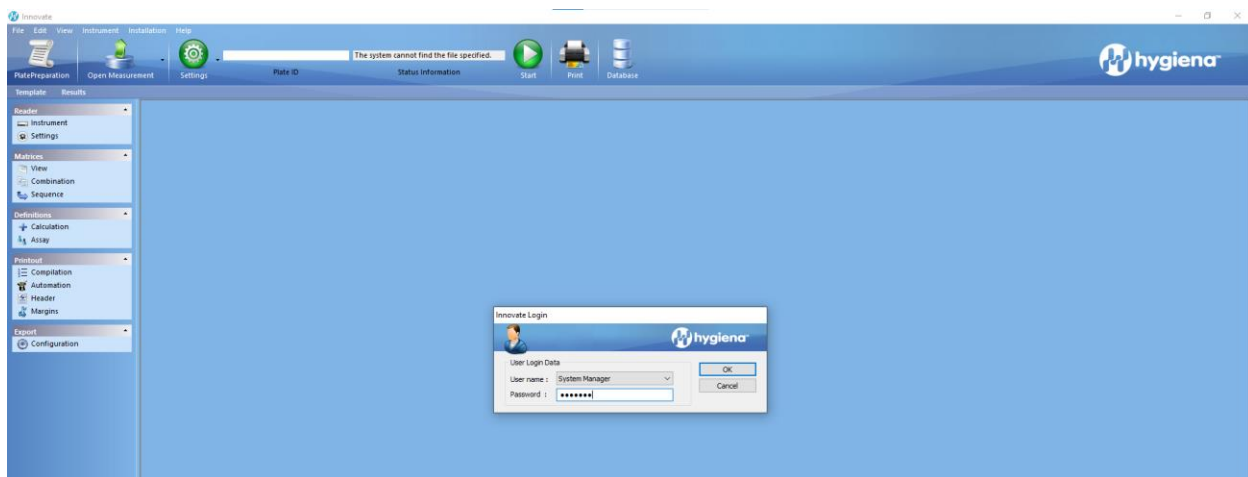


3. Change password to **Default1**. Click OK

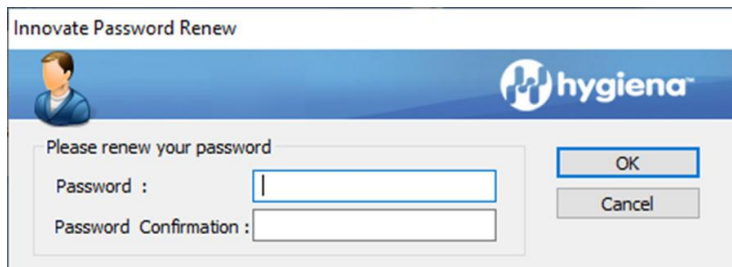


4. Go to **Assay** under **Definitions**, highlight **Product** and click **duplicate**.




5. NewTst1 will show up on the screen. **Highlight** NewTst1 and click **Edit**

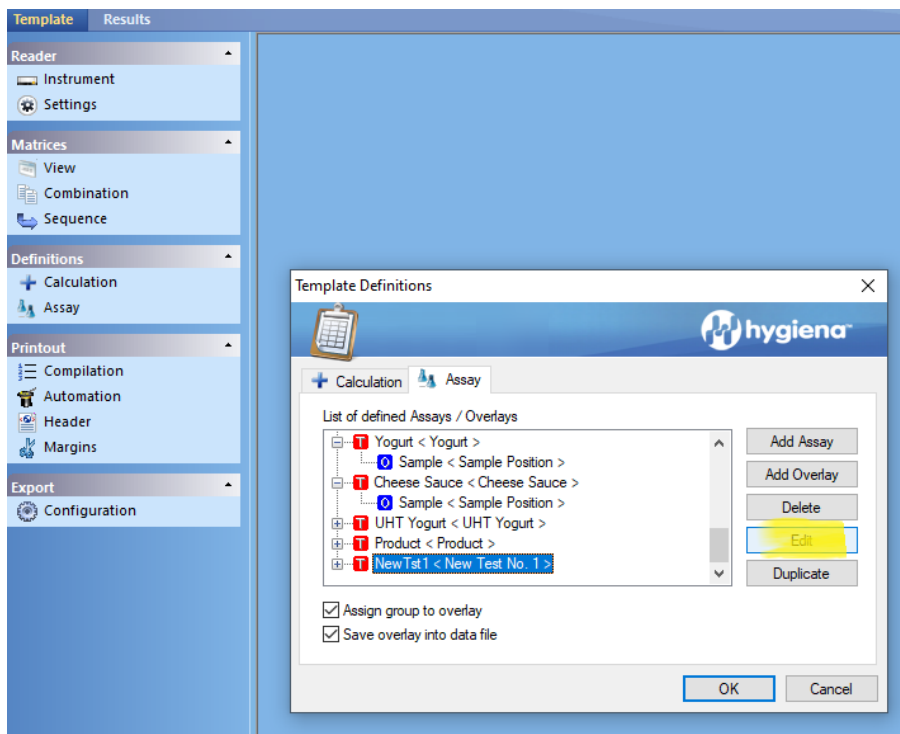


6. Under **General Information**, edit assay name and assay description based on client preference. In this example, WPS was inputted to represent Whey Protein Shake

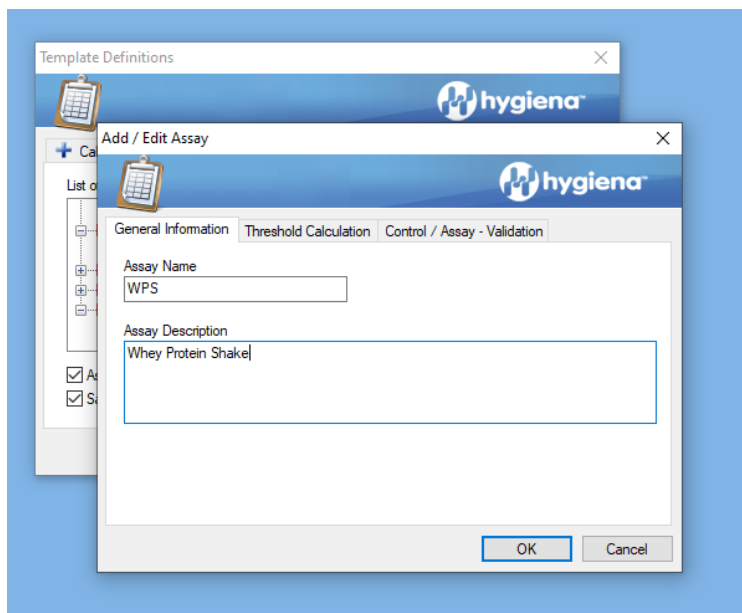

7. Go to **Threshold Calculation Tab** to set negative and positive thresholds after performing RLU baseline study. In this example, anything less than or equal to 25 RLU is considered negative, whereas anything more than or equal to 26 RLU is considered positive. Click **OK**.

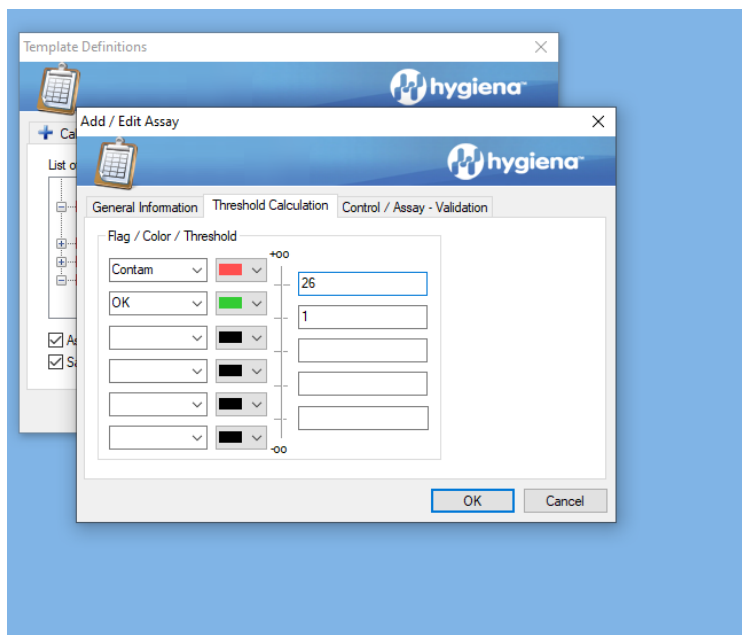


8. Notice that NewTst1 has been changed to an assigned name. Click **OK**.



9. Notice that the protocol name has changed in the lower right corner of the software screen.



10. Go to **File** at the top left hand corner, go to **Template** to bring up this screen.



11. **Highlight** RS\_Dairy and click **Save As** to bring up this screen.

New Template Name

Please enter a new name for the template

RS\_Dairy\_New

OK Cancel

12. Enter in new RS\_Dairy protocol name, making sure to only add to the end of the name and not replace RS\_Dairy. Click **OK** when finished. Example below.

New Template Name

Please enter a new name for the template

RS\_Dairy1

OK Cancel

13. Go to **File → Template** and open your new template file you just saved by highlighting the new protocol and selecting **Open**

Template Results

Reader

- Instrument
- Settings

Matrices

- View
- Combination
- Sequence

Definitions

- Calculation
- Assay

Printout

- Compilation
- Automation
- Header
- Margins

Export

- Configuration

Template

hygiena

Template	Access	Date Modified	User
RS_Dairy	ReadOnly	2020-04-28 17:30:18	Hygiena
RS_Dairy1	Customize	2021-04-30 10:19:08	System Manager
RS_Dairy_Control	ReadOnly	2020-04-28 17:30:38	Hygiena
RS_Injector_Test	ReadOnly	2020-04-28 17:30:58	Hygiena

Open Save Save as ... Delete OK

14. You can confirm your new protocol is saved and loaded by checking the **Assay** tab as shown below. In this example, our WPS product appears!

